

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0030
Location:	DEAL POLICE	
Calibration File No.:	00834	Calib. Date: 09/14/2018
Certification File No.:	00835	Cert. No.: 00028
Linearity File No.:	00836	Cert. Date: 09/14/2018
Solution File No.:	00881	Lin. No.: 00025
Sequential File No.:	00881	Lin. Date: 09/14/2018
		Soln. No.: 00186
		Soln. Date: 01/12/2019
		File Date: 01/12/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0039
Solution Control Lot:	18290	Expires: 09/17/2020
		Bottle No.: 0534

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:18S		
Control 1 EC	-.---%	18:19S	33.9°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	18:19S	33.9°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

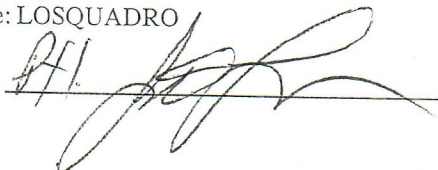
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LOSQUADRO

First Name: JONATHAN

MI: L

Signature: 

Badge No.: 130

Date: 01/12/2019