

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWM-0030  
Location: DEAL POLICE  
Calibration File No.: 00925 Calib. Date: 07/17/2019 Calib. No.: 00030  
Certification File No.: 00926 Cert. Date: 07/17/2019 Cert. No.: 00027  
Linearity File No.: 00927 Lin. Date: 07/17/2019 Lin. No.: 00028  
Solution File No.: 00938 Soln. Date: 11/02/2019 Soln. No.: 00201  
Sequential File No.: 00938 File Date: 11/02/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0039  
Control Solution %: 0.100% Expires: 02/11/2021  
Solution Control Lot: 19060 Bottle No.: 0571

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:48S		
Control 1 EC	0.100%	15:48S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:49S		
Control 2 EC	0.100%	15:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:50S		
Control 3 EC	0.100%	15:51S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:52S		

All tests within acceptable tolerance.

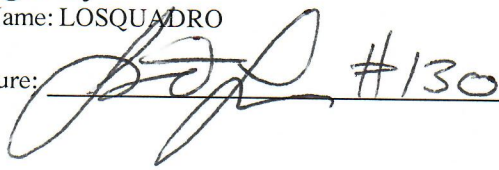
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: LOSQUADRO

First Name: JONATHAN

MI: L

Signature:  #130

Badge No.: 130

Date: 11/02/2019