

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWM-0030  
Location: DEAL POLICE  
Calibration File No.: 00925 Calib. Date: 07/17/2019 Calib. No.: 00030  
Certification File No.: 00926 Cert. Date: 07/17/2019 Cert. No.: 00027  
Linearity File No.: 00927 Lin. Date: 07/17/2019 Lin. No.: 00028  
Solution File No.: 00934 Soln. Date: 09/29/2019 Soln. No.: 00199  
Sequential File No.: 00934 File Date: 09/29/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0039  
Control Solution %: 0.100% Expires: 02/11/2021  
Solution Control Lot: 19060 Bottle No.: 0578

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:56D		
Control 1 EC	0.100%	05:57D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:57D		
Control 2 EC	0.100%	05:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	05:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:59D		
Control 3 EC	0.100%	05:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: SHARIN

First Name: MATTHEW

MI: J

Signature: \_\_\_\_\_

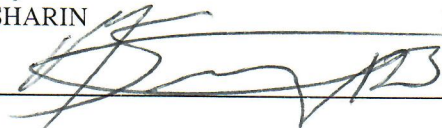

Badge No.: 123

Date: 09/29/2019