

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0030
Location:	DEAL POLICE	Calib. Date:	06/29/2020
Calibration File No.:	00969	Calib. No.:	00032
Certification File No.:	00970	Cert. Date:	06/29/2020
Linearity File No.:	00971	Lin. Date:	06/29/2020
Solution File No.:	00991	Soln. Date:	10/21/2020
Sequential File No.:	00991	File Date:	10/21/2020
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	4
Solution Control Lot:	20390	Expires:	09/02/2022
		Bottle No.:	1433

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:40D		
Control 1 EC	0.100%	15:41D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:42D		
Control 2 EC	0.099%	15:42D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:43D		
Control 3 EC	0.099%	15:44D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:44D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LOSQUADRO

First Name: JONATHAN

MI: L

Signature: _____

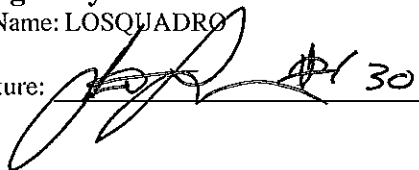

Badge No.: 130

Date: 10/21/2020