

Calibrating Unit

New Standard Solution Report

| | | | |
|-------------------------|-----------------------|--------------|------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARWM-0030 |
| Location: | DEAL POLICE | | |
| Calibration File No.: | 00969 | Calib. Date: | 06/29/2020 |
| Certification File No.: | 00970 | Cert. No.: | 00032 |
| Linearity File No.: | 00971 | Lin. Date: | 06/29/2020 |
| Solution File No.: | 00993 | Cert. No.: | 00029 |
| Sequential File No.: | 00993 | Lin. No.: | 00030 |
| | | Soln. Date: | 11/15/2020 |
| | | Soln. No.: | 00227 |
| | | File Date: | 11/15/2020 |
| | | | |
| Calibrating Unit: | WET | Model No.: | CU-34 |
| Control Solution %: | 0.100% | Serial No.: | 4 |
| Solution Control Lot: | 20390 | Expires: | 09/02/2022 |
| | | Bottle No.: | 1473 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|-----------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 23:19S | | |
| Control 1 EC | -.---% | 23:20S | 33.9°C | CTRL GAS SUPPLY |
| Control 1 IR | -.---% | 23:20S | 33.9°C | CTRL GAS SUPPLY |
| Ambient Air Blank | -.---% | --:-- | | |
| Control 2 EC | -.---% | --:-- | N/A | |
| Control 2 IR | -.---% | --:-- | N/A | |
| Ambient Air Blank | -.---% | --:-- | | |
| Control 3 EC | -.---% | --:-- | N/A | |
| Control 3 IR | -.---% | --:-- | N/A | |
| Ambient Air Blank | -.---% | --:-- | | |

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LOSQUADRO

First Name: JONATHAN

MI: L

Signature: _____

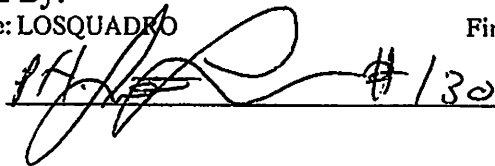

Badge No.: 130

Date: 11/15/2020