

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0030
Location:	DEAL POLICE		
Calibration File No.:	00995	Calib. Date:	11/30/2020
Certification File No.:	00996	Cert. Date:	11/30/2020
Linearity File No.:	00997	Lin. Date:	11/30/2020
Solution File No.:	01007	Soln. Date:	02/09/2021
Sequential File No.:	01007	File Date:	02/09/2021
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0038
Solution Control Lot:	20390	Expires:	09/02/2022
		Bottle No.:	0231

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:49S		
Control 1 EC	0.096%	11:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	11:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51S		
Control 2 EC	0.097%	11:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	11:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:52S		
Control 3 EC	0.097%	11:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54S		

All tests within acceptable tolerance.

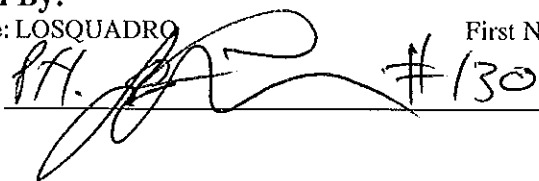
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: LOSQUADRO

First Name: JONATHAN

MI: L

Signature:  #130

Badge No.: 130

Date: 02/09/2021