

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDXAS3-0039

Certification Date:

Technician:

Re-Certification Due Date:

2.24.21

DM

2.24.22

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

Certification Date:

Next Certification Due:

DDUNP2-466

2.24.21

2.24.22

Probe Value:

102

Draeger, Inc.

DM

Alcotest 7110 Calibration Record


Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0030
Location:	DEAL POLICE		
Calibration File No.:	01020	Calib. Date:	05/25/2021
Certification File No.:	00996	Cert. No.:	00034
Linearity File No.:	00997	Cert. Date:	11/30/2020
Solution File No.:	01017	Lin. Date:	11/30/2020
Sequential File No.:	01020	Lin. No.:	00031
		Soln. Date:	05/11/2021
		Soln. No.:	00239
		File Date:	05/25/2021
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0039
Solution Control Lot:	19270	Expires:	10/14/2021
		Bottle No.:	0008

Coordinator

Last Name: LUTZ First Name: DENNIS MI: J
Signature: Tpi I dent 7045 Badge No.: 7045
Date: 05/25/2021

*Black Key Temperature Probe Serial.....# DDLBP3-0115 (DC)

*Digital NIST Temperature Measuring System Serial.....# 200 357 843 (DC)

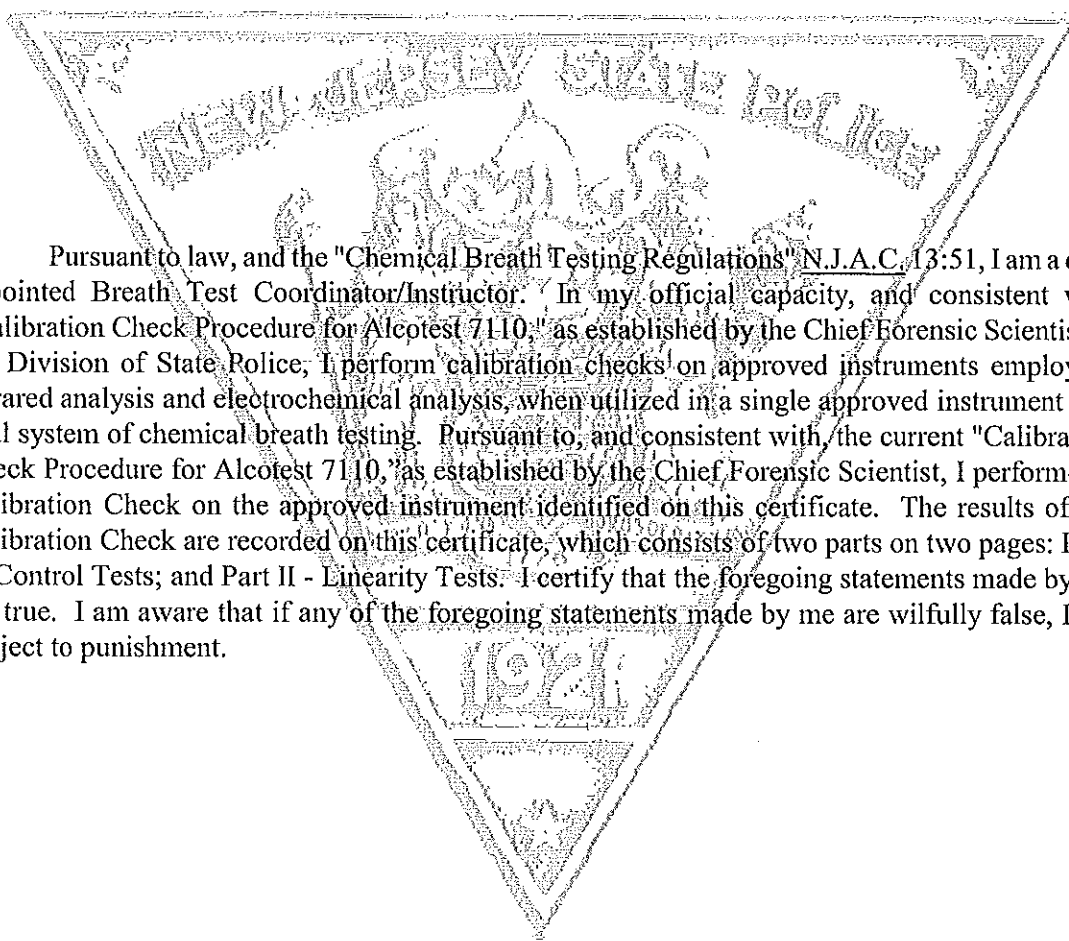

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0030
Location: DEAL POLICE
Calibration File No.: 01020 Calib. Date: 05/25/2021 Calib. No.: 00034
Certification File No.: 01021 Cert. Date: 05/25/2021 Cert. No.: 00031
Linearity File No.: 00997 Lin. Date: 11/30/2020 Lin. No.: 00031
Solution File No.: 01017 Soln. Date: 05/11/2021 Soln. No.: 00239
Sequential File No.: 01021 File Date: 05/25/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0039
Control Solution %: 0.100% Expires: 10/14/2021
Solution Control Lot: 19270 Bottle No.: 0008

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:30D		
Control 1 EC	0.100%	09:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31D		
Control 2 EC	0.100%	09:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33D		
Control 3 EC	0.100%	09:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:35D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: _____

Badge No.: 7045

Date: 05/25/2021

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0030
Location: DEAL POLICE
Calibration File No.: 01020 Calib. Date: 05/25/2021 Calib. No.: 00034
Certification File No.: 01021 Cert. Date: 05/25/2021 Cert. No.: 00031
Linearity File No.: 01022 Lin. Date: 05/25/2021 Lin. No.: 00032
Solution File No.: 01017 Soln. Date: 05/11/2021 Soln. No.: 00239
Sequential File No.: 01022 File Date: 05/25/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0005
Control Solution %: 0.040% Expires: 11/04/2021
Solution Control Lot: 19310 Bottle No.: 1267

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0211
Control Solution %: 0.080% Expires: 11/11/2021
Solution Control Lot: 19320 Bottle No.: 0541

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0005
Control Solution %: 0.160% Expires: 12/02/2021
Solution Control Lot: 19360 Bottle No.: 0211

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:50D		
Control 1 EC	0.040%	09:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	09:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52D		
Control 2 EC	0.040%	09:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	09:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55D		
Control 3 EC	0.081%	09:56D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57D		
Control 4 EC	0.081%	09:58D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59D		
Control 5 EC	0.160%	10:00D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.158%	10:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02D		
Control 6 EC	0.159%	10:03D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.158%	10:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: _____

Top I Lutz 7045

Badge No.: 7045

Date: 05/25/2021

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0030
Location: DEAL POLICE
Calibration File No.: 01020 Calib. Date: 05/25/2021 Calib. No.: 00034
Certification File No.: 01021 Cert. Date: 05/25/2021 Cert. No.: 00031
Linearity File No.: 01022 Lin. Date: 05/25/2021 Lin. No.: 00032
Solution File No.: 01023 Soln. Date: 05/25/2021 Soln. No.: 00240
Sequential File No.: 01023 File Date: 05/25/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0039
Control Solution %: 0.100% Expires: 01/13/2023
Solution Control Lot: 21010 Bottle No.: 0991

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:13D		
Control 1 EC	0.102%	11:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		
Control 2 EC	0.102%	11:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:16D		
Control 3 EC	0.101%	11:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DOWNPZ-466 (DC)

Changed By:

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: Tpc I Dent 7045

Badge No.: 7045

Date: 05/25/2021

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Tpr I Dennis J Lutz
Name

7045
Badge No.

Location:

Dept. Police
Agency

ALYM-0030
Alcotest Serial No.

Equipment:

200 357 843
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDMKS3-0005	08:16 D	09:17 D	33.9°C
0.08%	DOWES3-0211	08:16 D	09:18 D	33.9°C
0.10%	DDXA53-0039	08:16 D	09:19 D	33.9°C
0.16%	DDSC53-0005	08:16 D	09:20 D	33.8°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr I Lutz 7045
Coordinator's Signature

5-25-21
Date

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDMKS3-0005

Certification Date:

3.18.21

Technician:

NPB

Re-Certification Due Date:

3.18.22

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDWES3-D211

Certification Date:

3.18.21

Technician:

NPB

Re-Certification Due Date:

3.18.22

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDSCS3-0005

Certification Date:

3.19.21

Technician:

[Signature]

Re-Certification Due Date:

3.19.22

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDLBP3-0115

Certification Date:

3.25.21

Next Certification Due:

3.25.22

Probe Value:

102

Draeger, Inc. [Signature]



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11349797

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 200357843 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Thermistor Module	A27129	04 Feb 2021	1000451212
Temperature Calibration Bath	A42238		
Temperature Calibration Bath	B01375		
Temperature Probe	5394	21 Feb 2021	C0220030
Temperature Calibration Bath	B16388		
Temperature Probe	5267	21 Feb 2021	C0220028
Temperature Calibration Bath	B3A444		
Thermistor Module	B96381	16 Jul 2020	B9626028
Temperature Probe	5398	16 Jul 2020	B9605083
Thermistor Module	B96382	19 Aug 2020	B9628006
Temperature Probe	5410	13 Sep 2020	B9801031

Certificate Information:

Technician: 420 Procedure: CAL-06 Cal Date: 15 Jun 2020 Cal Due Date: 15 Jun 2022
 Test Conditions: 52.44%RH 23.46°C 1018mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.001	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.001	25.001	Y	24.951	25.051	0.0087	>4:1
°C	N.A.	N.A.		50.002	50.001	Y	49.952	50.052	0.0087	>4:1
°C	N.A.	N.A.		100.001	99.998	Y	99.951	100.051	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement: (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±((Max-Min)/2); Min=As Left Nominal/Rounded) - Tolerance; Max= As Left Nominal/Rounded) + Tolerance;

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Marisa Elms
Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
 Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
 International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11349797

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 15 Jun 2020

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/21/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1232 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 14, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of October, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/14/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19310

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 04, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of November, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 6/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/20/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19320

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0971 to 0.0985 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 11, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of November, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 12/11/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1956 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 02, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18 day of December, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recycle





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 01/28/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21010

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 13, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29 day of January, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Dennis J. Lutz

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1946 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 29th DAY OF January

TWO THOUSAND AND Nineteen


J. P. Kelly
COLONEL
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 07/11)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Dennis J. Lutz
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF


THE LAWS OF 1946 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 1st DAY OF October

TWO THOUSAND AND Nine


J. P. Kelly
COLONEL
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2-7-11	OCPA	Wm. Hon
2. 1/24/13	OCPA	Adam Stender
3. 11-23-15	OCPA	M. Gonzalez
4. 4/6/17	LAKELAND	Adam Stender
5. 8/22/19	NDSP Galloway	Bill
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 07/11)

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 68 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date

12-6-16

SERIAL NUMBER

ARWM-0030

Draeger Safety Diagnostics, Inc.

BC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDXAS3-0039

Certification Date:

2.24.21

Technician:

DM

Re-Certification Due Date:

2.24.22

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months

of the certification date below, or sooner, according to your state's specifications.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDUNP2-466

Certification Date:

2.24.21

Next Certification Due:

2.24.22

Probe Value:

102

Dräger, Inc.

DM