

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0030
Location:	DEAL POLICE		
Calibration File No.:	01020	Calib. Date:	05/25/2021
Certification File No.:	01021	Cert. No.:	00034
Linearity File No.:	01022	Lin. Date:	05/25/2021
Solution File No.:	01045	Cert. No.:	00031
Sequential File No.:	01045	Lin. No.:	00032
		Soln. Date:	10/24/2021
		Soln. No.:	00245
		File Date:	10/24/2021
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0039
Solution Control Lot:	21010	Expires:	01/13/2023
		Bottle No.:	0988

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:06D		
Control 1 EC	-.---%	21:07D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	21:07D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DOWLING

First Name: NICHOLAS

MI: C

Signature: _____

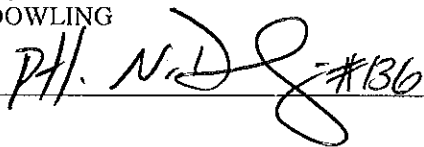

Badge No.: 136

Date: 10/24/2021