

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWM-0030  
Location: DEAL POLICE  
Calibration File No.: 01048 Calib. Date: 11/12/2021 Calib. No.: 00035  
Certification File No.: 01049 Cert. Date: 11/12/2021 Cert. No.: 00032  
Linearity File No.: 01050 Lin. Date: 11/12/2021 Lin. No.: 00033  
Solution File No.: 01063 Soln. Date: 01/24/2022 Soln. No.: 00252  
Sequential File No.: 01063 File Date: 01/24/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0038  
Control Solution %: 0.100% Expires: 01/13/2023  
Solution Control Lot: 21010 Bottle No.: 1406

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:54S		
Control 1 EC	0.099%	13:55S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:56S		
Control 2 EC	0.099%	13:57S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:58S		
Control 3 EC	0.099%	13:59S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:59S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:00S		

All tests within acceptable tolerance.

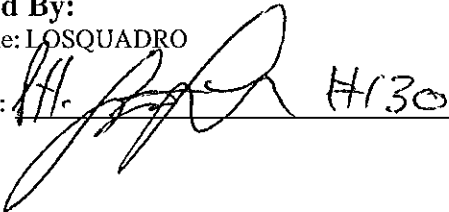
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: LOSQUADRO

First Name: JONATHAN

MI: L

Signature:  H130

Badge No.: 130

Date: 01/24/2022