

Sgt. Kevin Alcott #6704
Alcotest Project Manager
Alcohol Drug Testing Unit
New Jersey State Police
1200 Negron Drive - Suite 400
Hamilton, NJ 08691
Cell: 609-218-3345
Email: kevin.alcott@njsp.org



ALCOTEST 9510 PARAMETER REPORT

Equipment

Serial No.: ARMH-0005
 Firmware: 8326739 1.5
 WinCE application: 8326738 2.9
 Configuration: 8326737 3.10

Date: 06/08/2022
 Time: 13:12:32

Parameter

min. blow time	5.0	s
min. breath volume for females of age 60+	1.2	L
min. breath volume for all other	1.5	L
min. blow flow	4.5	L/min
plateau detection limit	4	%
plateau detection start conc.	70	microgram/L
neg. flow detection (part. vacuum)	10.0	hPa
neg. flow detection sensitivity	10	
cal. gas abort volume	0.4	L
result-to-zero limit	0.0050	%BAC
ambient air check limit	0.0049	%BAC
interference det. d-criterion limit abs.	38	microgram/L
interference det. d-criterion limit rel.	10.0	%
interference det. t-criterion limit abs.	8	microgram/L
interference det. t-criterion limit rel.	2.1	%
IR CO2 offset	10	microgram/L
IR H2O offset	4	microgram/L
EC H2O offset	0	microgram/L
Value-based EC aging comp. on/off (1/0)	0	
Time-based EC aging comp. on/off (1/0)	1	
Time-based EC aging comp. per month	0.2	%
Time-based EC aging comp. maximum	3.0	%
EC fatigue comp. max. sum	15000	
EC fatigue comp. factor	50	
EC fatigue comp. minutes	180	
mouth alc. mark limit	500	
mouth alc. lower limit	30	
mouth alc. slope	6	
mouth alc. zero limit	50	
mouth alc. max. neg. sum	6	
mouth alc. max. 2nd derivative	35	

ALCOTEST 9510 CERTIFICATION REPORT - WET ADJUST (PART I)
Deal Borough

Equipment

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0005
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

Wet Adjust Record

Wet Adjust File No.: 25 Wet Adjust Date: 06/08/2022 Wet Adjust No.: 1
Wet Adjust Time: 14:43:58

Concentration: 0.100 %
Adjusting Unit: X-Cal 2000 Adj. Unit Ser. No.: ARND-0001 Adj. Unit Exp.: 01/13/2023
Solution Lot No.: 21210 Soln. Bottle No.: 64 Adjust Soln. Exp.: 06/16/2023

Preadjust Simulator Temp.: 34.00 degree C
Postadjust Simulator Temp.: 34.01 degree C

Result

Procedure completed successfully.

Coordinator

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

Sgt K A 6704

Signed:

Date: 06/08/2022

ID: 1

ALCOTEST 9510 CERTIFICATION REPORT - DRY ADJUST (PART II)
Deal Borough

Equipment

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0005
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

Dry Adjust Record

Dry Adjust File No.: 26 Dry Adjust Date: 06/08/2022 Dry Adjust No.: 1
Dry Adjust Time: 14:57:14

Concentration: 0.100 %
Dry Gas Lot No.: 1460885 Adjust Gas Exp.: 03/12/2024
Barom. Model No.: Mensor CPG2300 Barom. Serial No.: 41001270 Barom. Cert. Exp.: 12/01/2022
Pre-adjust Amb. Pressure: 1012 hPa Post-adjust Amb. Pressure: 1010 hPa

Result

Procedure completed successfully.

Coordinator

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

Sgt. K A 6704

Signed:

Date: 06/08/2022

ID: 1

ALCOTEST 9510 CERTIFICATION REPORT - LINEARITY (PART III)
Deal Borough

Equipment

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0005
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

Linearity Record

Linearity File No.: 27 Lin. Date: 06/08/2022 Lin. No.: 1

0.040% Dry Gas Lot No.: 1486624 Adjust. Gas Exp.: 04/26/2024
 0.080% Dry Gas Lot No.: 1346773 Adjust. Gas Exp.: 07/08/2023
 0.160% Dry Gas Lot No.: 1523726 Adjust. Gas Exp.: 07/16/2024
 0.300% Dry Gas Lot No.: 1495468 Adjust. Gas Exp.: 05/14/2024

Data Summary

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	15:02:49		*TEST PASSED*
Control .04 Test 1 EC	0.039	15:03:27	1010	*TEST PASSED*
Control .04 Test 1 IR	0.039	15:03:27	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:04:23		*TEST PASSED*
Control .04 Test 2 EC	0.040	15:04:37	1010	*TEST PASSED*
Control .04 Test 2 IR	0.039	15:04:37	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:05:59		*TEST PASSED*
Control .08 Test 3 EC	0.078	15:06:35	1010	*TEST PASSED*
Control .08 Test 3 IR	0.079	15:06:35	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:07:36		*TEST PASSED*
Control .08 Test 4 EC	0.080	15:07:51	1010	*TEST PASSED*
Control .08 Test 4 IR	0.080	15:07:51	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:10:03		*TEST PASSED*
Control .16 Test 5 EC	0.155	15:10:41	1010	*TEST PASSED*
Control .16 Test 5 IR	0.159	15:10:41	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:11:47		*TEST PASSED*
Control .16 Test 6 EC	0.158	15:12:02	1010	*TEST PASSED*
Control .16 Test 6 IR	0.160	15:12:02	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:13:30		*TEST PASSED*
Control .30 Test 7 EC	0.290	15:14:06	1010	*TEST PASSED*
Control .30 Test 7 IR	0.297	15:14:06	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:15:21		*TEST PASSED*
Control .30 Test 8 EC	0.295	15:15:35	1010	*TEST PASSED*
Control .30 Test 8 IR	0.300	15:15:35	1010	*TEST PASSED*
Ambient Air Blank	0.000	15:16:00		*TEST PASSED*

Result

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

Sgt. K A 6704

Signed:

Date: 06/08/2022

ID: 1

ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 1
Deal Borough
SERIAL NUMBER: ARMH-0005

Equipment

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0005
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9
Cyl1 Install File No.: 28 Cyl1 Install Date: 06/08/2022 Cyl1 Install No.: 1

Control Tests (0.100%)

Installation Inlet: #1 (Upper) Post test active Cyl.: #1 (Upper)
Dry Gas Lot No.: 1507099 Dry Gas Lot Exp.: 06/11/2024

Data Summary

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	15:20:42		*TEST PASSED*
Control Test 1			1010	*TEST PASSED*
EC Result	0.098	15:21:28		*TEST PASSED*
IR Result	0.100	15:21:28		*TEST PASSED*
Ambient Air Blank	0.000	15:22:32		*TEST PASSED*
Control Test 2			1010	*TEST PASSED*
EC Result	0.099	15:22:57		*TEST PASSED*
IR Result	0.100	15:22:57		*TEST PASSED*
Ambient Air Blank	0.000	15:24:02		*TEST PASSED*
Control Test 3			1009	*TEST PASSED*
EC Result	0.100	15:24:27		*TEST PASSED*
IR Result	0.100	15:24:27		*TEST PASSED*
Ambient Air Blank	0.000	15:24:52		*TEST PASSED*

Result

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

Sgt. *KA* 6704

Signed:

Date: 06/08/2022

ID: 1

ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 2
Deal Borough
SERIAL NUMBER: ARMH-0005

Equipment

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0005
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9
 Cyl2 Install File No.: 29 Cyl2 Install Date: 06/08/2022 Cyl2 Install No.: 1

Control Tests (0.100%)

Installation Inlet: #2 (Lower) Post test active Cyl.: #2 (Lower)
 Dry Gas Lot No.: 1507099 Dry Gas Lot Exp.: 06/11/2024

Data Summary

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	15:28:25		*TEST PASSED*
Control Test 1			1009	*TEST PASSED*
EC Result	0.098	15:29:10		*TEST PASSED*
IR Result	0.100	15:29:10		*TEST PASSED*
Ambient Air Blank	0.000	15:30:15		*TEST PASSED*
Control Test 2			1009	*TEST PASSED*
EC Result	0.099	15:30:39		*TEST PASSED*
IR Result	0.100	15:30:39		*TEST PASSED*
Ambient Air Blank	0.000	15:31:44		*TEST PASSED*
Control Test 3			1009	*TEST PASSED*
EC Result	0.099	15:32:08		*TEST PASSED*
IR Result	0.101	15:32:08		*TEST PASSED*
Ambient Air Blank	0.000	15:32:33		*TEST PASSED*

Result

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

Sgt. K A 6704

Signed:

Date: 06/08/2022

ID: 1



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/07/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21210

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1199 to 0.1215 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 16, 2023.


As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of July, 2021.

Notary

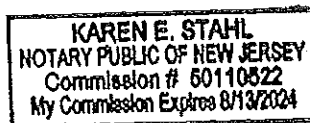


An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Customer: DRAEGER INC
7256 S SAM HOUSTON PKWY W
STE 100
HOUSTON, TX 77085
PO Number: S1O4302598632

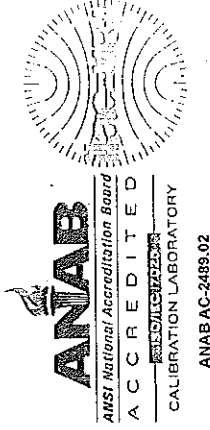

Certificate/SO Number: 5-D6Z1H-60-1 Revision 0

Manufacturer: Drager Safety AG & Co. KGaA
Model Number: X-Cal 2000
Description: Breath Alcohol Simulator
Serial Number: ARND-0001
ID: NONE

As-Found: In Tolerance
As-Left: In Tolerance
Issue Date: Jan 13, 2022
Calibration Date: Jan 13, 2022
Due Date: Jan 13, 2023

Calibrated To: Customer Specification
Calibration Procedure: 1-AC103519-1

Transcat Calibration Laboratories have been audited and found in compliance with ISO IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/NCSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS 16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/NCSL Z540.3-2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor k=2, providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-1B. For mass calibrations: Conventional mass referenced to 6.0 g/cm³.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

Customer: DRAEGER INC
 7256 S SAM HOUSTON PKWAY W
 STE 100
 HOUSTON, TX 77085
 PO Number: S1O4302598632



Certificate/SO Number: 5-D6Z1H-60-1 Revision 0

Description	Setpoints	Accuracy	As Found/As Left Data			Units	TUR
			Low Limit	High Limit	As Found / As Left		
Function Checks							
Bubble Check			P	P	P		
Seal Check			P	P	P		
Temperature Source: Accuracy Test							
Accuracy Test	34.00°C	±(0.02 °C)	33.98	34.02	34.01 °C	1.1e-002	1.6e-002 °C
Temperature Source: Stability Test							
Stability Test	0.00°C	±(0.02 °C)	-0.02	0.02	0.00 °C	1.1e-002	1.6e-002 °C

Field not applicable.

Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
05H1277	AccuMac Corporation	AM1760-12-S	Secondary SPRT	27-May-21	31-May-22	15-805H1277-3-1	AF/AL
HP927312	Hart Scientific/Fluke	1575	Super Thermometer	18-May-21	30-Nov-22	5-8HP927312-5-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings; AL - used for as-left readings.

Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
70.52°F /21.40°C	36.80%	Dew/K6	G	Temperature

Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal

Customer: DRAEGER INC
7256 S SAM HOUSTON PKWY W
STE 100
HOUSTON, TX 77085
PO Number: S1O4302598632



Certificate/SO Number: 5-D6Z1H-60-1 Revision 0

to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

Customer: DRAEGER INC
7256 S SAM HOUSTON PKWY W
STE 100
HOUSTON, TX 77085
PO Number: S1O4302598632



Certificate/ISO Number: 5-D6Z1H-60-1 Revision 0

Legend

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique Identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

CALIBRATED
BY **TRANSCAT**

CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC
7256 S SAM HOUSTON PKWY W
STE 100
HOUSTON, TX 77085
PO Number: S1O4302598632



Certificate/SO Number: 5-D6Z1H-60-1 Revision 0

Calibrated At:
16115 Park Row
Houston, TX 77084

Facility Responsible:
16115 Park Row
Houston, TX 77084
800-828-1470

Unit Barcode: **0900B4365**
0900B43653

Date Received: January 12, 2022
Service Level: R9

Calibrated By: Camden Alford
Calibration Technician
Jan 13, 2022 12:41:00 -05:00

Reviewed By: Josh Solbeau for
Electronically Signed By:
Jan 13, 2022 14:06:08 -05:00


Certificate - Page 5 of 5
Reprinted on January 19, 2022

Customer Number: 1-659111-000
OPS-F20-014R10 09/29/21 FP001R9 4/9/2021

CALIBRATED BY TRANSCAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC
7256 S SAM HOUSTON PKWY W
STE 100
HOUSTON, TX 77085
PO Number: S104302546536

Certificate/SO Number: 5-GG5JD-40-1 Revision 0

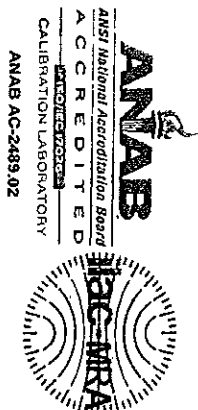

Manufacturer: Wika Instr/Mensor Corp/Trend
Model Number: CPG2300
Description: Portable Barometer
Serial Number: 41001270
ID: NONE

As-Found: In Tolerance
As-Left: In Tolerance
Issue Date: Dec 01, 2021
Calibration Date: Dec 01, 2021
Due Date: Dec 01, 2022

Calibrated To: Manufacturer Specification
Calibration Procedure: 1-AC107288-0

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/NCSL Z540-1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSINCSL Z540-3-2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.


Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor $k=2$, providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm³.

The results in this report relate only to the item calibrated or tested. Recorred calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturer's (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

CALIBRATED BY TRANSAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC
 7256 S SAM HOUSTON PKWY W
 STE 100
 HOUSTON, TX 77085
 PO Number: S104302546536

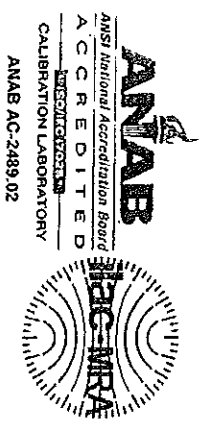

Certificate/ISO Number: 5-GG5JD-40-1 Revision 0


As Found/As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	Cal Process Uncertainty (k=2; ±)	Measurement Uncertainty (k=2; ±)	Units	TUR
Pressure Measure: 552 to 1172 mbara Range									
550.1mbara	±(0.015% FS)	549.9	550.3	550.1 mbara	1.0e-002	1.2e-001	mbara	19.1 : 1	
610.0mbara	±(0.015% FS)	609.8	610.2	610.0 mbara	1.2e-002	1.2e-001	mbara	17.3 : 1	
680.4mbara	±(0.015% FS)	680.2	680.6	680.4 mbara	1.3e-002	1.2e-001	mbara	15.5 : 1	
734.3mbara	±(0.015% FS)	734.1	734.5	734.3 mbara	1.4e-002	1.2e-001	mbara	14.3 : 1	
804.7mbara	±(0.015% FS)	804.5	804.9	804.6 mbara	1.5e-002	1.2e-001	mbara	13.1 : 1	
864.9mbara	±(0.015% FS)	864.7	865.1	864.9 mbara	1.6e-002	1.2e-001	mbara	12.2 : 1	
924.9mbara	±(0.015% FS)	924.7	925.1	924.9 mbara	1.8e-002	1.2e-001	mbara	11.4 : 1	
985.2mbara	±(0.015% FS)	985.0	985.4	985.2 mbara	1.9e-002	1.2e-001	mbara	10.7 : 1	
1043.9mbara	±(0.015% FS)	1043.7	1044.1	1043.9 mbara	2.0e-002	1.3e-001	mbara	10.1 : 1	
1114.2mbara	±(0.015% FS)	1114.0	1114.4	1114.2 mbara	2.1e-002	1.2e-001	mbara	9.4 : 1	
1174.6mbara	±(0.015% FS)	1174.4	1174.8	1174.6 mbara	2.2e-002	1.2e-001	mbara	9.0 : 1	
924.9mbara	±(0.015% FS)	924.7	925.1	924.9 mbara	1.8e-002	1.2e-001	mbara	11.4 : 1	
864.9mbara	±(0.015% FS)	864.7	865.1	864.9 mbara	1.6e-002	1.2e-001	mbara	12.2 : 1	
804.7mbara	±(0.015% FS)	804.5	804.9	804.6 mbara	1.5e-002	1.2e-001	mbara	13.1 : 1	

Field not applicable.

CALIBRATED BY TRANSICOT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC
 7256 S SAM HOUSTON PKWY W
 STE 100
 HOUSTON, TX 77085
 PO Number: S104302546536

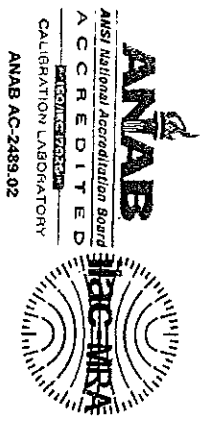

Certificate/ISO Number: 5-GG5JD-40-1 Revision 0

Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
DW11BA	Fluke/DH Instruments	PG7601	Piston Gauge	5-Apr-21	5-Apr-22	5-8DW11BA-10-1	AF/AL
DW11CA	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	3-Sep-21	3-Dec-21	5-8DW11CA-10-1	AF/AL
DW11LOW	Fluke/DH Instruments	PC-7100/7600-10-TC	Gas Piston-Cylinder Module	2-Mar-17	31-Mar-22	5-8DW11LOW-1-1	AF/AL
DW11MASS	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	4-Jun-20	31-Dec-21	5-8DW11MASS-4-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
71.57°F /21.98°C	47.20%	DewK5	B	Secondary Pressure


Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

CALIBRATED BY TRANSIST CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC
 7256 S SAM HOUSTON PKWY W
 STE 100
 HOUSTON, TX 77085
 PO Number: S104302546536

Certificate/SO Number: 5-GG5JD-40-1 Revision 0

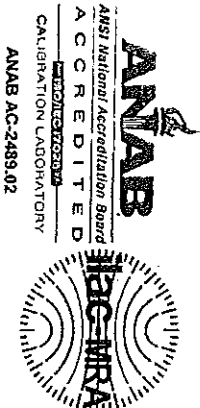


Topic	Description	Legend
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances	
As Found	Initial measurement results	
As Left	Measurement results after adjustment and/or repair	
Blank Data Field	Test is not applicable for the UUT	
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result	
Calibration Date	Indicates the date that the calibration was completed	
Cover Factor (K)	A measure of uncertainty that defines an interval about the measurement result	
Due Date	Indicates the end of the calibration cycle as requested by the customer	
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued	
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement	
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity	
OOA	Out of Acceptance (#)	
OOT	Out of Tolerance (*)	
Setpoints	Measurement target values	
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)	
Traceability Number	Unique Identifier(s) used to document traceability of calibration standards	
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results	
UUT	Unit Under test	

CALIBRATED BY TRANSCAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC
7256 S SAM HOUSTON PKWY W
STE 100
HOUSTON, TX 77085
PO Number: S104302546536

Certificate/SO Number: 5-GG5JD-40-1 Revision 0

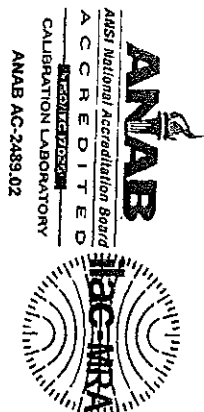


Calibrated At:
16115 Park Row
Houston, TX 77084


Facility Responsible:
16115 Park Row
Houston, TX 77084
800-828-1470

Unit Barcode: 
09008429641


Date Received: November 15, 2021
Service Level: R9

Calibrated By:
 Electronically Signed By:
Fritz Cardona

Fritz Cardona
Calibration Technician
Dec 01, 2021
09:27:49 -05:00

Reviewed By:
 Electronically Signed By:
Scott D. Caine

Scott D. Caine
Lab Manager
Dec 01, 2021
09:49:04 -05:00



CERTIFICATE OF ANALYSIS
EBS - ETHANOL BREATH STANDARD

DRAEGER, INC
1221 S. BELTLINE RD, STE 700
COPPELL TX 75019

INVOICE#: 20908188
PO#: US44302331960
CUST. ITEM #: 4401036
DATE: Mar. 19, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.
CALGAZ LOT#: 1460885
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: Mar. 12, 2024

Table with 3 columns: COMPONENT, PPM, (BrAC). Rows include ETHANOL (260.5, 0.100), NITROGEN (BAL), AVERAGE ANALYTICAL VALUE, and ETHANOL (262.8, 0.101).

Table with 3 columns: REFERENCE STANDARD, CYLINDER, CONCENTRATION PPM. Row: N.M.I. TRACEABLE STANDARDS*, ND50144, 260.6

* CERTIFICATION TRACEABLE TO National Metrology Institute Traceable Standards.

TRACEABILITY

Preparation:
Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44, Calibration test 121088, 121097, 121091, or 121100 dated, 18th January 2019 applies.

Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.
Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650

No affecting environmental conditions during analysis.

*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: Mar. 12, 2021

CALGAZ CYLINDER SIZE: 6D

APPROVED BY : [Signature]

"We certify that all the cylinders for the lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

ANALYSIS CERTIFICATION

METHOD OF PREPARATION : GRAVIMETRIC / PRESSURE TRANSFILLING

METHOD OF ANALYSIS : IR Breath Alcohol Analyzer

ACCURACY : ± 0.002 BrAC or $\pm 2\%$ whichever is greater.

LOT NO. & QTY.	COMP. 1 C ₂ H ₅ OH	COMP. 2 N ₂	COMP. 3	COMP. 4	COMP. 5	COMP. 6	Exp Date
1486624 (8)	104.2PPM						04/26/24
	(0.040 BrAC) BALANCE						

TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited Company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

WEIGHT SETS USED: Kit#80141, Test#3094344A, Kit#106, 27, 103, 107, 113, 22, Test#VA-21-12587-L,F,T,P, Kit#IM1966, Test#VA-21-12587N, Kit#35, 104, 39, 105, 108, 109, 111 Test#VA-21-12587-I.

No affecting environmental conditions during analysis.

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

REQUESTED BY : DRAEGER INC

CUSTOMER PURCHASE ORDER NUMBER : US44302368647

PACKING LIST NUMBER : 21272590

CERTIFICATION DATE : April 26, 2021

ANALYSIS BY : Steven Blutschek
Quality Representative

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC
821 Chesapeake Drive, Cambridge, MD 21613-0149
Phone: (410)228-6400 Fax: (410)228-4251

ANALYSIS CERTIFICATION

METHOD OF PREPARATION : GRAVIMETRIC / PRESSURE TRANSFILLING

METHOD OF ANALYSIS : IR Breath Alcohol Analyzer

ACCURACY : ± 0.002 BrAC or $\pm 2\%$ whichever is greater.

LOT NO. & QTY.	COMP. 1 C ₂ H ₅ OH	COMP. 2 N ₂	COMP. 3	COMP. 4	COMP. 5	COMP. 6	Exp Date
1346773 (24)	208.4PPM (0.080 BrAC) BALANCE						07/08/23

TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited Company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 121088, 121097, 121091, or 121100 dated, 18th January 2019 applies.

WEIGHT SETS USED: Kit #92231, Test #2740564, Kit # 03610, Test # VA-19-1135 T3 Test # VA-19-11350B, T5 Test #VA-19-11350F, VA-19-11350E, VA-19-11350D, IM1966 Test VA-18-11340H

No affecting environmental conditions during analysis.

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

REQUESTED BY : DRAEGER INC

CUSTOMER PURCHASE ORDER NUMBER : UH54302105642

PACKING LIST NUMBER : 16572762

CERTIFICATION DATE : July 8, 2020

ANALYSIS BY : Staver Plutschal
Quality Representative

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC
821 Chesapeake Drive, Cambridge, MD 21613-0149
Phone: (410)228-6400 Fax: (410)228-4251

CERTIFICATE OF ANALYSIS
EBS - ETHANOL BREATH STANDARD

DRAEGER INC HOUSTON
HOUSTON, TX 77085

REF#: 22053560
DOC#: US44302425104
CUST. ITEM #: 4401040
DATE: Jul. 16, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.
CALGAZ LOT#: 1523726
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: Jul. 16, 2024

COMPONENT	PPM	(BrAC)
ETHANOL	416.8	(0.160)
NITROGEN	BAL	

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND50144	260.6

* Certification traceability is recognized by NIST through the CIPM MRA.

TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650


No affecting environmental conditions during analysis.

*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: Jul. 16, 2021

CALGAZ CYLINDER SIZE: 6D

APPROVED BY : 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC
821 Chesapeake Drive, Cambridge, MD 21613-0149
Phone: (410)228-6400 Fax: (410)228-4251

CERTIFICATE OF ANALYSIS
EBS - ETHANOL BREATH STANDARD

DRAEGER INC HOUSTON
HOUSTON, TX 77085

REF#: 21766042
DOC#: US44302404557
CUST. ITEM #: 4401041
DATE: Jun. 11, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.
CALGAZ LOT#: 1495468
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: May. 14, 2024

COMPONENT	PPM	(BrAC)
ETHANOL	781.5	(0.300)
NITROGEN	BAL	

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND50144	260.6

* Certification traceability is recognized by NIST through the CIPM MRA.

TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650


No affecting environmental conditions during analysis.

*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: May. 14, 2021

CALGAZ CYLINDER SIZE: 6D

APPROVED BY : 

"We certify that all the cylinders for the lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC
821 Chesapeake Drive, Cambridge, MD 21613-0149
Phone: (410)228-6400 Fax: (410)228-4251

CERTIFICATE OF ANALYSIS
EBS - ETHANOL BREATH STANDARD

DRAEGER INC HOUSTON
HOUSTON, TX 77085

REF#: 21775557
DOC#: US44302405855
CUST. ITEM #: 4401036
DATE: Jun. 18, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.
CALGAZ LOT#: 1507099
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: Jun. 11, 2024

COMPONENT	PPM	(BrAC)
ETHANOL	260.5	(0.100)
NITROGEN	BAL	

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND50144	260.6

* Certification traceability is recognized by NIST through the CIPM MRA.

TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.
Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

Analytical:


Analytical Instruments Calibrated Using NMI Traceable Standards.
Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650

No affecting environmental conditions during analysis.

*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: Jun. 11, 2021

CALGAZ CYLINDER SIZE: 6D

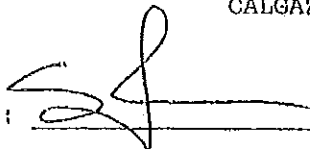APPROVED BY : 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC
821 Chesapeake Drive, Cambridge, MD 21613-0149
Phone: (410)228-6400 Fax: (410)228-4251

CERTIFICATE OF ANALYSIS
EBS - ETHANOL BREATH STANDARD

DRAEGER INC HOUSTON
HOUSTON, TX 77085

REF#: 21775557
DOC#: US44302405855
CUST. ITEM #: 4401036
DATE: Jun. 18, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.
CALGAZ LOT#: 1507099
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: Jun. 11, 2024

COMPONENT	PPM	(BrAC)
ETHANOL	260.5	(0.100)
NITROGEN	BAL	

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND50144	260.6

* Certification traceability is recognized by NIST through the CIPM MRA.

TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.
Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.
Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650

No affecting environmental conditions during analysis.

*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: Jun. 11, 2021

CALGAZ CYLINDER SIZE: 6D

APPROVED BY : 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC
821 Chesapeake Drive, Cambridge, MD 21613-0149
Phone: (410)228-6400 Fax: (410)228-4251



Dräger

Alcotest 9510

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

5/31/2022

ARMH-0005

Draeger, Inc. CR

DEPARTMENT OF
Water and Public Safety
 This is to certify that

Kevin W. Alcott

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1986 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION,
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One

[Signature]
 COLONEL
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2338 (Rev. 01/18)

DEPARTMENT OF
Water and Public Safety
 This is to certify that

Kevin W. Alcott

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1986 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION,
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One

[Signature]
 COLONEL
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2338 (Rev. 01/18)

Dräger

Alcotest 9510

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

5/31/2022

ARMH-0005

Draeger, Inc. _____

CR